3050 Spruce Street, St. Louis, MO 63103 USA
Tel: (800) 521-8956 (314) 771-5765 Fax: (800) 325-5052 (314) 771-5757
email: techservice@sial.com sigma-aldrich.com

Product Information

Codeine solution 1.0 mg/mL±5% in methanol drug standard

Catalog Number **C1653** Lot Number 088K8752 Storage Temperature 2–8 °C

CAS RN 76-57-3

Synonyms: $(5\alpha,6\alpha)$ -7,8-Didehydro-4,5-epoxy-3-methoxy-17-methylmorphinan-6-ol; Methymorphine;

Morphine monomethyl ether

Product Description

Molecular Formula: C₁₈H₂₁NO₃ Molecular Weight: 299.36

DEA Class: Exempt preparation of Class II

Concentration: 0.97 mg of codeine/mL of GC grade methanol, concentration verified by UV.

Expiration Date: September 2010

Precautions and Disclaimer


This product is for R&D use only, not for drug, household, or other uses. Please consult the Material Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

Store the product at 2–8 $^{\circ}$ C. If stored at 2–8 $^{\circ}$ C in an airtight container, protected from light, decomposition of the product is less than 1% in 24 months. After opening, concentration may change due to loss of solvent.


CMW,MAM 09/08-1

70 eV Electron Ionization Mass Spectrum

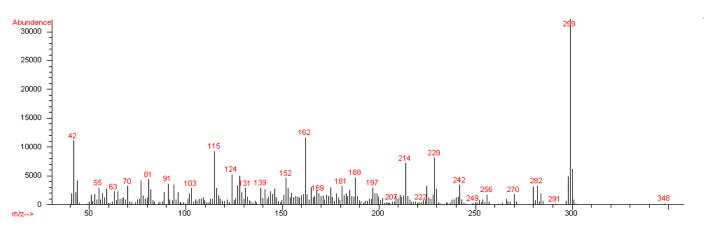

Hewlett-Packard 5890 Series II Gas Chromatograph Hewlett-Packard 5971 Mass Selective Detector Hewlett-Packard G1034C MS ChemStation (HP-DOS series)

FT-IR

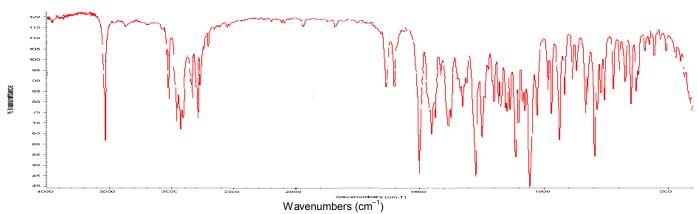


Nicolet Magna IR Spectrometer Series II


Ultraviolet Spectrum

Peak	284.0 nm
Absorbance	0.6213
Solvent	0.2 N H ₂ SO ₄
Dilution	1:9 (v/v)

Capillary Gas Chromatography

Column Supelco SPB-1 (Catalog Number 24162)
I.D. 0.20 mm Length 15 m Film Thickness 0.20 μm
Oven Temperature 150 °C (2 minutes), then
15 °C/minute to 300 °C, hold 18 minutes
Injector Temperature 250 °C, Split
Detector Hewlett-Packard 5971
Mass Selective Detector (70 eV, 40-500 m/z)

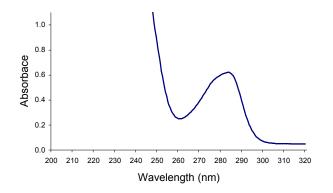

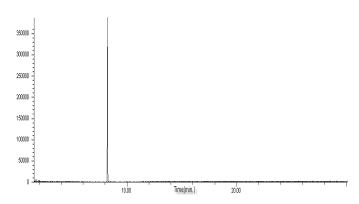

Beckman-Coulter DU-800

Hewlett-Packard 5890