

**User Manual**

# **GenElute™ -E Single Spin Plant DNA Kit**

For Purification of Genomic DNA from Plant Samples

**EC500**

**Sigma-Aldrich®**

What's Inside:

**Introduction** ..... 2  
 Reduced waste for a better environment  
 A simplified workflow

**Intended Use** ..... 4  
 Typical Results

**Storage and Stability** ..... 5  
 Kit Storage  
 Sample Storage and Variability  
 Disposal

**Materials and Equipment Needed** ..... 5  
 Kit Contents  
 Not Supplied in Kit  
 Preparation before starting

**Standard Protocol** ..... 6  
 Lysis  
 Column Preparation  
 Purification of DNA

**Cap Puncher Protocol** ..... 7  
 Lysis  
 Column Preparation  
 Purification of DNA

**Troubleshooting** ..... 8


**Product Ordering** ..... 10  
 Precautions and Disclaimer  
 Notice  
 Standard Warranty  
 Contact Information  
 Technical Assistance

**GenElute™-E Single Spin Checklist** ..... 11  
 EC500

For research use only.

## Introduction

GenElute™-E Single Spin Kits are a nucleic acid purification system that eliminates the need for high salt binding and ethanol wash steps, yielding DNA and RNA preparations with fewer impurities for more robust results. GenElute™-E DNA and RNA purification kits employ a **negative chromatography** method dependent on size exclusion to separate large DNA and RNA nucleic acid molecules from smaller protein, lipid, and ionic components in cell, tissue, blood, and other samples.

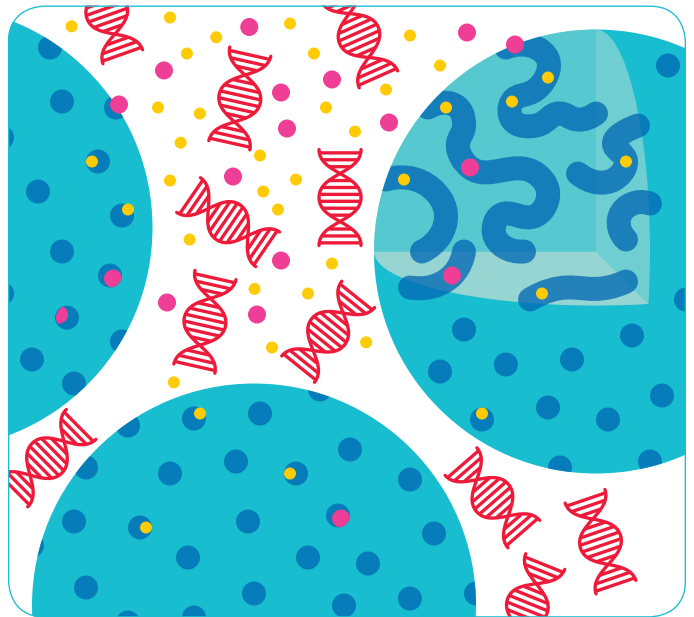



Using negative chromatography, Single Spin columns efficiently absorb and retain sample contaminants while allowing nucleic acids to flow through the column, reducing the number of steps and plastic materials required for purification. The key is the novel lysis that allows negative chromatography to be used for high quality nucleic acid purification.

Three key advantages over silica:

- Simplified workflow
- Superior performance
- Waste reduction

## A simplified workflow

Purification in one spin, eliminating all wash steps and reducing tube handling for more efficient, safer sample processing.

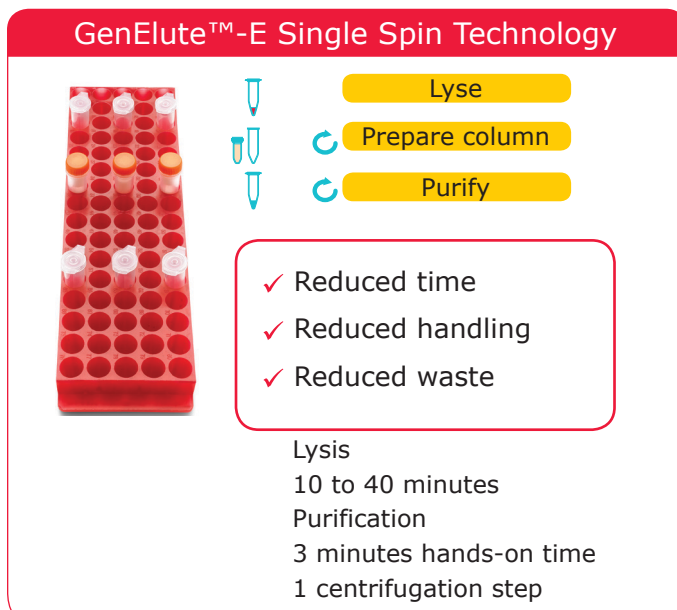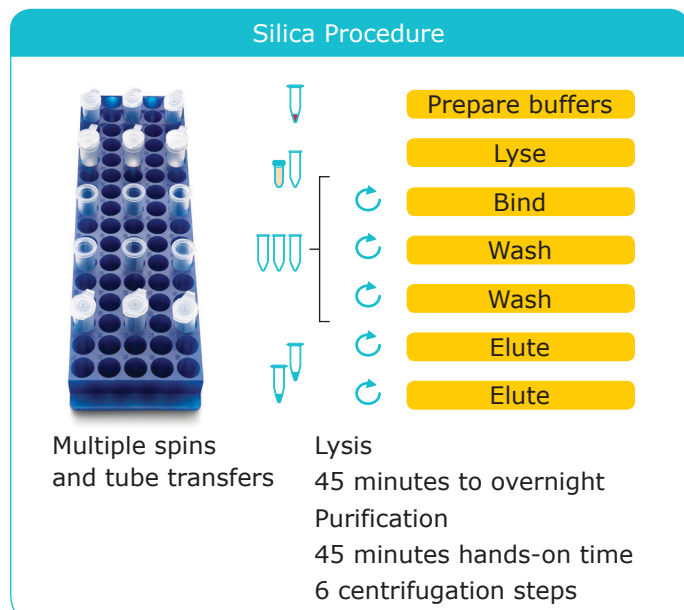

## Reduced waste for a better environment

With fewer plastic tubes and no hazardous liquids, GenElute™-E DNA and RNA purification kits provide an eco-friendly alternative to silica-based purification.

GenElute™-E purification kits greatly reduce the amounts of plastic-based components packaged with each kit and consumed while executing protocols in the lab. All tedious binding and washing steps associated with silica-based procedures are omitted, with no use of hazardous materials such as chaotropic salts or organic solvents that require special disposal. Plastic waste is reduced by 55% compared to a common silica kits, resulting in disposal cost savings and reduced environmental impact.

GenElute™-E Single Spin nucleic acid purification kits provide easier workflows for DNA and RNA isolation, better nucleic acid quality with fewer impurities, and reduced plastic and hazardous waste disposal compared to silica bind-wash-elute spin prep kits.

### GenElute™-E Single Spin Purification supports:

- Significantly reduced plastic waste
- No hazardous bind and wash steps
- Responsible and sustainable nucleic acid purification
- Disposal cost savings



## Specifications

Sample Input	10 – 50 mg
Sample Type	plant tissues like leaves, blossoms, fruits, roots, flour and seed samples
Sample Condition	Fresh, frozen, dried
Required time after lysis	2 minutes
Purified Nucleic Acid	DNA > 200 bp
Elution Volume	90-110 µl
The purified genomic DNA is ready for immediate use in downstream applications:	<ul style="list-style-type: none"> <li>• Restriction digestions</li> <li>• PCR and qPCR</li> <li>• Southern blots</li> <li>• Sequencing reactions</li> </ul>

## Intended Use

For Single Step purification of genomic DNA from plant tissue samples. This protocol has been developed for 10–50 mg plant tissues like leaves, blossoms, fruits, roots, flour and seed samples. 30 mg is generically recommended (for certain plant species, optimization of input amount may be required).


## Typical Results

**Table 1**

Sample Type	Typical Yield µg/10mg	Sample Type	Typical Yield µg/10mg
cucumber leaf	2-10	nicotiana leaf	1-5
parsley leaf	5-50	potato leaf	1-5
basil leaf	5-15	melon leaf	2-10
tomato leaf	1-5	pepper leaf	5-10
apple leaf	1-5	cauliflower leaf	2-10
kiwi leaf	1-5	tomato fruit	0.5-2
quince leaf	5-15	leek fruit	2-10
morello cherry leaf	1-5	avocado fruit	1-5
lettuce leaf	0.5-2	tulip petal	1-5
lemon leaf	1-5	garlic	5-45
petunia leaf	0.5-2	ginger	1-5
orchid leaf	0.5-2	onion	1-5
pine needle	0.1-0.5	rape root	0.5-1
leek leaf	1-5	wheat	0.5-1
arabidopsis leaf	0.5-2	lentils	1-5
spinach leaf	2-10	barley	0.1-1
		pumpkin seed	5-10
		walnut	2.5-5

Typical yields reflect µg of gDNA per 10mg of initial sample. Due to sample variability, results may vary.

**Figure 1**

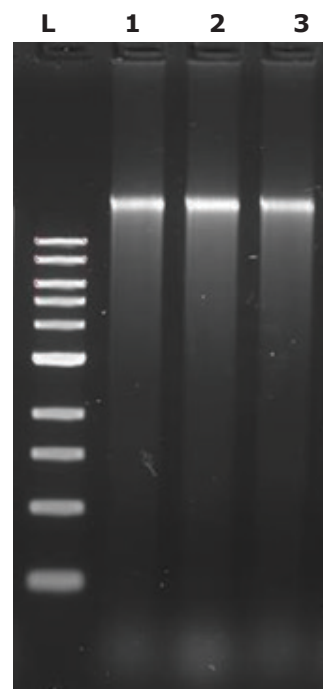

Spectrophotometric results of three replicates of gDNA isolation from 7.5 mg of lentils per isolation using GenElute™-E Single Spin Plant DNA Kit. Gel electrophoresis shown in Figure 1. Due to sample variability, results may vary.

	Replicate 1	Replicate 2	Replicate 3
<b>Concentration (ng/µl)</b>	48.90	43.20	28.80
260/280	1.97	1.82	1.84
260/230	2.23	2.16	2.13
Volume (µl)	96.00	101.00	94.00
Mass (ng)	4694.40	4363.20	2707.20
Average Mass (ng)	3921.6		



## Storage and Stability

### Kit Storage

Store SmartLyse™ P Protease **P** and RNase A Plant **R** at 2-8 °C. The remaining components should be stored at room temperature. Use the kit within 12 months of receipt.

### Sample Storage and Variability

Nucleic acid degrades over time, potentially leading to reduced fragment length and overall yield. Therefore, it is best if samples are acquired from fresh material. Often when working with samples, this is not feasible. Stabilizing the sample through the addition of stabilizing reagents and/or by immediately freezing the sample and storing it at -20°C or -70°C can assist in improving results.

However, it is important to keep in mind that individual samples are not homologous during collection and samples often vary between different plant species as well as among different parts of the plant itself. Plant cells are surrounded by cell walls that ensure mechanical stability of plant cell tissues. Due to the high mechanical resistance, a physical disruption of plant tissues before continuation of additional lytic steps is mandatory.

### Disposal

GenElute™-E kits adhere to the principles of "SMASH Packaging", our plan that drives improvement in the sustainability of our packaging through less packaging, more sustainable materials and easier recycling.

The box and insert material comes from sustainably managed forests and/or more than 70% of recycled content. The kit component bags are composed of starch-based, compostable material. Please recycle.

Kit components exposed to samples should be disposed of with biological waste. Other kit materials should be disposed of according to all applicable international, federal, state, and local regulations.

## Materials and Equipment Needed

### Kit Contents

- Plant Lysis Buffer **LB**
- SmartLyse™ P Protease **P**
- Grinding Solution **GS**
- Clearing Solution P **CS**
- RNase A Plant **R**
- 1x Tris Buffer **T**
- Spin Columns **●**

### Not Supplied in Kit

- Microcentrifuge with rotor for 1.5 mL and 2 mL reaction tubes.

**Important:** Set centrifuge to relative centrifugal force, rcf (x g). If needed, calculate equivalent rpm by the formula:

$$\text{rpm} = 1,000 \times \sqrt{g / (1.12 \times r)},$$

where r = radius of rotor in mm  
and g is the required g-force.

- Thermal shaker with agitation, capable of heating to 60 °C and 80 °C.  
*Alternative: Heating Block or heat chamber.*
- Vortex device.
- Pipets for 10 µL and 200 µL scales, corresponding pipet tips.
- One reaction tube (1.5 mL) per sample for the lysis step.
- One reusable reaction tube (2 mL) per sample for column preparation.
- One reaction tube (1.5 mL) per sample for collection of the purified DNA.
- GenElute™-E Cap Puncher (optional)

### Preparation before starting

- Heat the thermal shaker or heating block/chamber to 60 °C.
- Set the microcentrifuge to 1,000 x g.

## Standard Protocol

### Lysis

1. Add 10 – 50 mg of plant tissue sample to reaction tube.
2. For each sample, transfer 100 µL Plant Lysis Buffer **LB**.

**Note:** If sample type is strongly absorbing liquid (e.g. freeze-dried material, some seeds), the amount of added Lysis Buffer needs to be increased to 200 µL.

3. Pulse vortex to resuspend Grinding Solution **GS** and add 10 µL to each reaction tube.
4. Add 2 µL RNase A Plant **R** to each reaction tube.
5. Homogenize plant tissue until completely disrupted.
6. Add 5 µL SmartLyse™ P Protease Mix **P** to a 1.5 mL reaction tube. Vortex briefly
7. Place the reaction tube(s) in the thermal shaker and incubate at 60 °C for 30 minutes with maximum agitation.

*If using Heating Block or heat chamber, vortex halfway through incubation time to re-suspend, and return to incubation.*

*Meanwhile during lysis, proceed with "Column Preparation".*

8. After incubation at 60 °C, increase the temperature to 80 °C and incubate for additional 10 minutes with maximum agitation.
9. After having performed lysis, add 25 µL Clearing Solution P **CS** to each sample and vortex for 3 seconds. The sample will become cloudy.
10. Centrifuge for 2 minutes at maximum speed.

### Column Preparation

11. Vortex the Spin Column briefly and place into a 2 mL reaction tube.


Let stand for 10 to 20 minutes.

12. Loosen the screw cap of the Spin Column and snap off bottom closure of the column. The screw cap must stay loosened half a turn to avoid generation of a vacuum. Place the Spin Column back into the 2 mL reaction tube.
13. Centrifuge for 1 minute at 1,000 x g. Discard the 2 mL reaction tube containing the column buffer.
14. Place the prepared Spin Column into a new 1.5 mL reaction tube for collection of the purified DNA and place back into the rack.

### Purification of DNA

15. Transfer a maximum of 100 µL of lysis supernatant containing the DNA into the prepared Spin Column as illustrated:

Open cap and pipet the sample slowly (5 sec) onto the center of the resin bed of the prepared Spin Column.



Close screw cap and loosen again half a turn.

**Important:** Do not re-close the screw cap of the Spin Column completely.



**Note:** During loading of lysate, do not touch the resin bed with your pipette tip. Residual cellular debris may be loaded and will not interfere with purification.

16. Centrifuge for 1 minute at 1,000 x g. The purified DNA flows through the column into the 1.5 mL storage tube. Discard the Spin Column.

The collected DNA can be used immediately or kept at 2-8 °C or for long-term storage at -20 °C. For spectrophotometric analysis, use the 1x Tris Buffer **T** supplied with the kit.

## Cap Puncher Protocol

### Lysis

1. Perform steps 1-10 from Standard Protocol.

### Column Preparation

11. Vortex the Spin Column briefly and place into a 2 mL reaction tube.
12. Let stand for 10 to 20 minutes.
13. Use of the Cap Puncher: Punch a hole into the column cap and lift the column together with the Cap Puncher out of the 2 mL collection tube. Snap off bottom closure of the column and detach the Cap Puncher by twisting clockwise while pulling out. Place the punched Spin Column back into the 2 mL reaction tube.
14. Centrifuge for 1 minute at 1,000 x g. Discard the 2 mL reaction tube containing the column buffer.
15. Place the prepared Spin Column into a new 1.5 mL reaction tube for collection of the purified DNA and place back into the rack.

### Purification of DNA


16. Transfer a maximum of 100  $\mu$ L of lysis supernatant containing the DNA into the prepared Spin Column as illustrated:


Insert pipet tip vertically through the hole in the column cap.

Pipet the sample slowly (5 seconds) into the column.

**Note:** Residual cellular debris may be loaded and will not interfere with purification.

17. Centrifuge for 1 minute at 1,000 x g. The purified DNA flows through the column into the 1.5 mL storage tube. Discard the Spin Column.

The collected DNA can be used immediately or kept at 2-8 °C or for long-term storage at -20 °C. For spectrophotometric analysis, use the 1x Tris Buffer  supplied with the kit.



## Troubleshooting

Problem	Probable Cause	Solution
	Individual samples have inherent variability. In addition, there is variability across different sample types. Optimization needs to be performed by the user to validate for their sample type.	Degraded DNA fragments below < 60 bp are depleted during purification. Using fresh samples stored under appropriate conditions or stabilizing the samples will help to mitigate low sample yields.
	Insufficient sample homogenization or sample shearing can decrease sample yield.	Optimize tissue disruption to minimize shearing of the nucleic acid. Visually inspect that the sample is completely homogenized before using with GenElute™-E kits.
	Using too much sample may result in overloading the column's capacity for separation.	Use the recommended sample load. Optimization needs to be performed by the user to validate for their sample type. A green tint to the purified sample is a key indicator with plant samples that the column was overloaded.
	Using too little of sample may result in low sample yields.	Use the recommended sample load. Optimization may need to be performed by the user if their sample type is low yielding.
Low yield	Small, possibly degraded, DNA-fragments (< 60 bp) and/or RNA (if RNase was used) are removed during purification. Since these components are co-purified with silica-based kits, there may be artificially lower oD 260 readings with GenElute™-E kits. Thus, the calculation of sample concentration and subsequent yield may appear lower.	Quantitation by measuring signal intensity of bands via gel electrophoresis fragment separation, using a fragment analyzer, or comparing qPCR Ct values will provide a more reliable measurement of full-length gDNA.
	Centrifugation speeds and spin times have been optimized to acquire the fraction of sample containing the nucleic acid.	Verify that centrifugation was performed under the recommended conditions.
	Incomplete lysis of the sample may lead to reduced yields. Lysis times may need to be extended depending on the sample type.	Additionally, the SmartLyse™ enzymes were optimized to work at the recommended temperature. Verify that the heating unit (ex. thermal shaker) is heating correctly.
	If the column preparation steps were performed incorrectly, then the separation resin will be packed incorrectly.	Verify that the preparation steps for the column were performed according to the protocol.
	When performing the Standard Protocol, without the use of the GenElute™-E Single Spin Cap Puncher, the cap may have been left untightened.	Verify that the spin column cap of the column is loosened half a turn to avoid vacuum generation.



Low sample volume	Loading too low of sample or too high of sample may result in sample volume loss. The loaded sample volume is required to be within the recommended range as that volume is required to displace the column buffer.	If the sample volume available to be loaded onto the column is below the recommended range, as may occur with dehydrated sample types, then bring the sample within the recommended range using lysis buffer. If the sample volume available to be loaded onto the column is above the recommended range, then only load up to the recommended volume.
	Blocking of pipette tips by lysate debris during aspiration of the supernatant may result in a lower transfer volume and, consequently, in a lower DNA yield.	Loading of debris onto the column will not impact the ability of the column to purify the nucleic acid from the sample. However, avoid aspirating the debris into the pipette tip or use wide-bore tips to aspirate if the sample has an abundance of debris to prevent clogging.
260/230 ratios appear to be "too low."	In some cases, the 260/230 ratios may be below the recommended range.	Downstream assays have not been shown to be compromised by lower 260/230 ratios using nucleic acid isolated using GenElute™-E kits.
RNA residues are observed.	If the optional RNase protocol is not performed, then there may be RNA observed.	Perform the optional RNase protocol. Some samples may require an extended incubation due to variability across sample types.
The purified sample has a green color.	Sometimes with plant samples the purified sample is green. In these cases, the column may be overloaded due to variations in sample type.	Reduce the amount of sample used with the kit.
Lysate leaks from the hole created by the Cap Puncher during loading	The sample needs to be loaded vertically, allowing the sample to be dispensed correctly into the column. Also, if there is not enough pressure applied using the Cap Puncher then the hole may not be large enough to load the sample.	Apply enough pressure using the Cap Puncher to create a hole and load sample vertically.
Columns with dried resin	In rare cases, the spin columns dry out during storage. This may be due to not storing the columns according to the recommended conditions.	Store GenElute™-E kits according to the recommended conditions.

## Product Ordering

Description	Qty	Catalogue No.
GenElute™-E Single Spin Blood DNA Kit	10	EC100-10RXN
	50	EC100-50RXN
	250	EC100-250RXN
GenElute™-E Single Spin Blood DNA High Yield Kit	10	EC200-10RXN
	50	EC200-50RXN
	250	EC200-250RXN
GenElute™-E Single Spin Tissue DNA Kit	10	EC300-10RXN
	50	EC300-50RXN
	250	EC300-250RXN
GenElute™-E Single Spin Cell Culture DNA Kit	10	EC400-10RXN
	50	EC400-50RXN
	250	EC400-250RXN
GenElute™-E Single Spin Plant DNA Kit	10	EC500-10RXN
	50	EC500-50RXN
	250	EC500-250RXN
GenElute™-E Single Spin DNA Cleanup Kit	10	EC600-10RXN
	50	EC600-50RXN
	250	EC600-250RXN
GenElute™-E Organic Solvent DNA Cleanup	10	EC700-10RXN
	50	EC700-50RXN
	250	EC700-250RXN
GenElute™-E Single Spin RNA Cleanup Kit	10	EC800-10RXN
	50	EC800-50RXN
	250	EC800-250RXN
GenElute™-E Tissue Stabilizer	100	EC111-100ML
	500	EC111-500ML
GenElute™-E RNA Gel Loading Buffer	1	EC222-1EA
	5	EC222-5EA
GenElute™-E Single Spin Tissue DNA 96 Kit	2	EC396-2EA
	8	EC396-8EA
GenElute™-E Single Spin Plant DNA 96 Kit	2	EC596-2EA
	8	EC596-8EA
GenElute™-E Single Spin Blood DNA 96 Kit	2	EC196-2EA
	8	EC196-8EA
GenElute™-E Single Spin Cap Puncher	1	EC9999-1EA

## Precautions and Disclaimer

This product is for research use only. Please consult the Safety Data Sheet for information regarding hazards and safe handling practices.

## Notice

We provide information and advice to our customers on application technologies and regulatory matters to the best of our knowledge and ability, but without obligation or liability. Existing laws and regulations are to be observed in all cases by our customers. This also applies in respect to any rights of third parties. Our information and advice do not relieve our customers of their own responsibility for checking the suitability of our products for the envisaged purpose.

The information in this document is subject to change without notice and should not be construed as a commitment by the manufacturing or selling entity, or an affiliate. We assume no responsibility for any errors that may appear in this document.

## Standard Warranty

The applicable warranty for the products listed in this publication may be found at [SigmaAldrich.com/terms](https://SigmaAldrich.com/terms).

## Contact Information

For the location of the office nearest you, go to [SigmaAldrich.com/offices](https://SigmaAldrich.com/offices).

## Technical Assistance

Visit the tech service page on our web site at [SigmaAldrich.com/techservice](https://SigmaAldrich.com/techservice).

MilliporeSigma, GenElute, SmartLyse and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.  
© 2022 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the U.S. and Canada.

# GenElute™-E Single Spin Checklist for Plant DNA Kit






## EC500

### Prepare before starting

- Heat the thermal shaker or heating block/chamber to 60 °C.
- Set the microcentrifuge to 1,000 x g.

### Lysis

- Add 10 – 50 mg of plant tissue to reaction tube.
- Add 100 µL Plant Lysis Buffer **LB**.
- Vortex to resuspend Grinding Suspension **GS**, add 10 µL.
- Add 2 µL RNase A Plant **R**. Vortex to mix.
- Homogenize sample.
- Add 5 µL SmartLyse™ P Protease Mix **P**.

Incubate  30 minutes  60 °C  10 minutes  80 °C  Thermal Shaker maximum agitation

- Add 25 µL Clearing Solution P **CS** and vortex shortly.
- Centrifuge 2 minutes at maximum speed.

### Column preparation (during 60 °C and 80 °C incubation)

- Vortex Spin Column and place in a 2 mL tube.
- Let stand for 20 minutes.



Loosen screw cap of Spin Column.

OR



Punch a hole in the cap with the GenElute™-E Single Spin Cap Puncher.

- Snap off bottom closure.
- Place Spin Column back into 2 mL tube.
- Centrifuge 1 minute at 1,000 x g to collect column buffer.
- Place column in a 1.5 mL tube.

### Purification of DNA

- Transfer lysate supernatant (maximum 100 µL).
- Centrifuge 1 minute at 1,000 x g to collect DNA.
- Collected DNA is ready to use.

Column prep during lysis