


## Product Information

### CODEINE

Methanol Solution


<b>Product Number</b>	C1653	<b>Synonyms</b>	(5 $\alpha$ ,6 $\alpha$ )-7,8-Didehydro-4,5-epoxy-3-methoxy-17-methylmorphinan-6-ol; Methymorphine; Morphine monomethyl ether
<b>Lot Number</b>	121K8804	<b>Stability</b>	If stored at 2-8°C in an air tight container, protected from light, decomposition of the product is less than 1% in 24 months. After opening, concentration may change due to loss of solvent.
<b>CAS Number</b>	[76-57-3]	<b>Expiration Date</b>	September 2004
<b>Concentration</b>	1.01 mg Codeine/mL GC grade methanol (conc. verified by UV)	<b>Storage</b>	2-8°C; After opening, transfer contents to small vial provided for your convenience.
<b>Molecular Formula</b>	C <sub>18</sub> H <sub>21</sub> NO <sub>3</sub>		
<b>Molecular Weight</b>	299.4		
<b>DEA Class</b>	Exempt preparation of Class II		

70 eV Electron Ionization Mass Spectrum

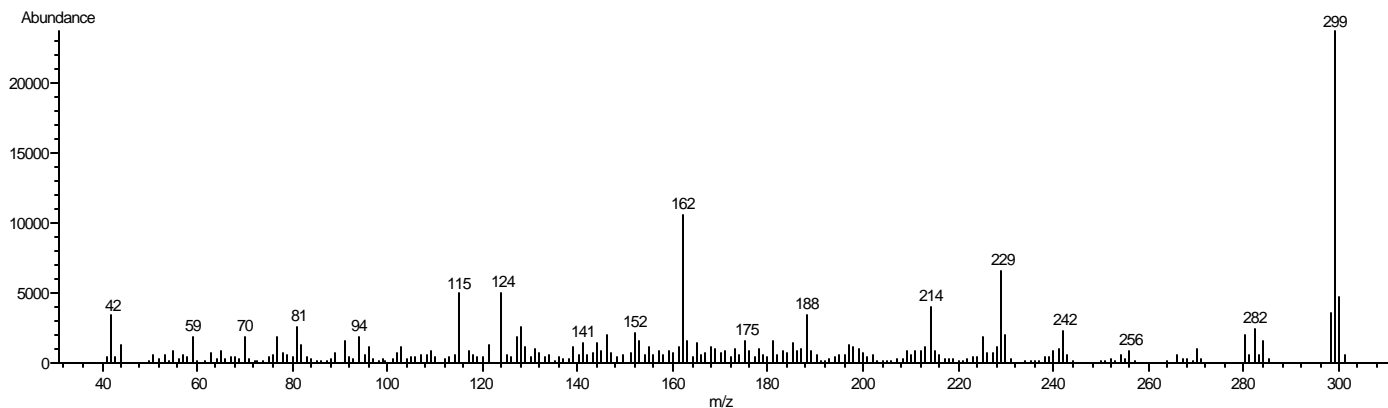


Hewlett-Packard 5890 Series II Gas Chromatograph  
 Hewlett-Packard 5971 Mass Selective Detector  
 Hewlett-Packard G1034C MS ChemStation (HP-DOS series)

### FT-IR

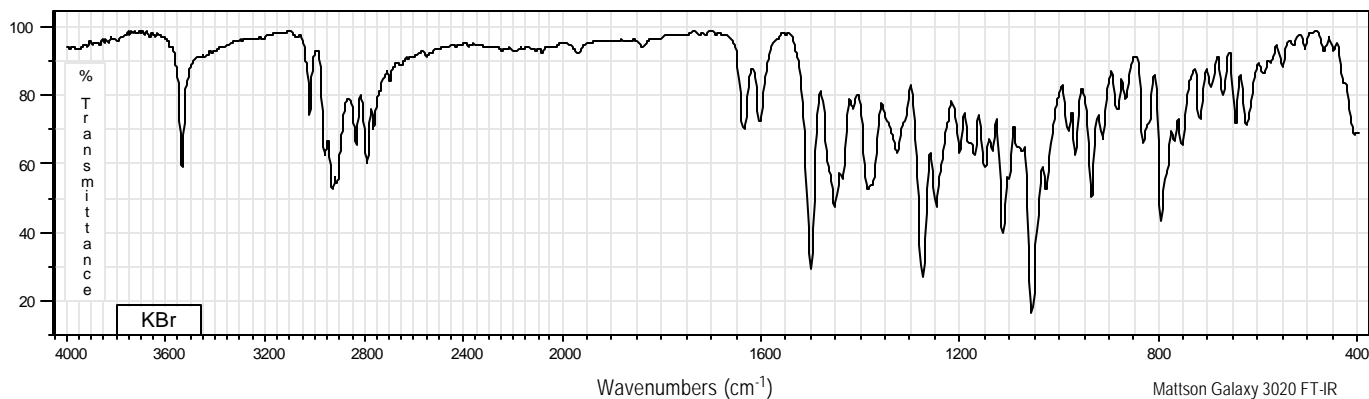


# CODEINE

Methanol Solution  
Product Number C 1653  
Lot Number 121K8804

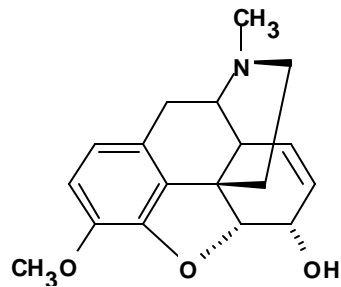

## Ultraviolet Spectrum


**Peak** 284.5 nm  
**Absorbance** 0.549  
**Solvent** 0.2 N H<sub>2</sub>SO<sub>4</sub>  
**Dilution** 1 : 9 (v/v)

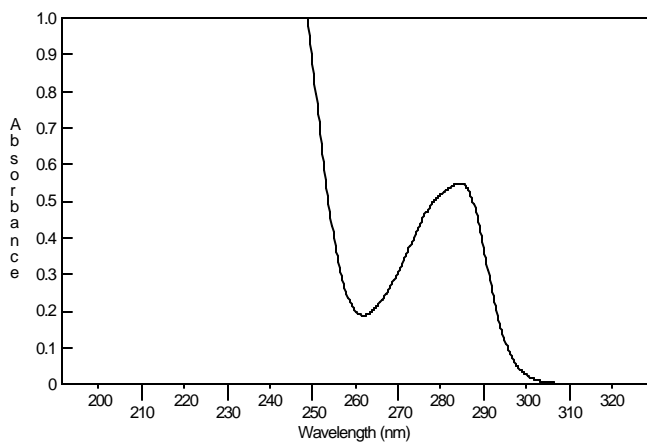

Bio-Tek Uvikon XL

## Capillary Gas Chromatography

**Column** Supelco SPB-1 (Cat. No. 2-4162)  
**I.D.** 0.20 mm **Length** 15 m **Film Thickness** 0.20 μm  
**Oven Temperature** 150°C (2 min.), then 15°/min. to 300°C, hold 18 min.  
**Injector Temperature** 250°C, Split  
**Detector** Hewlett-Packard 5971  
Mass Selective Detector (70 eV, 40-500 m/z)

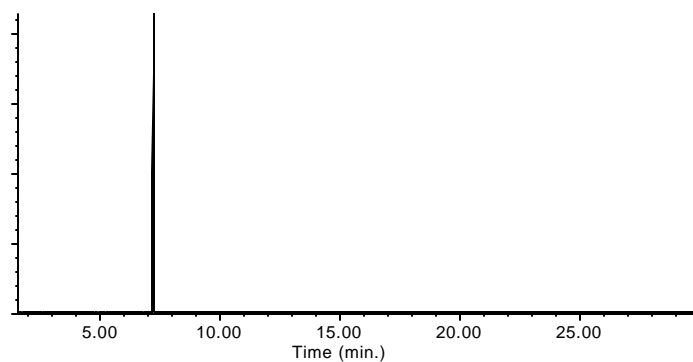

Hewlett-Packard 5890

C 1653/121K8804/01/15/02

This product is not for *in vitro* diagnostic procedures. For R&D use only. Not for drug, household or other uses.

Sigma brand products are sold through Sigma-Aldrich, Inc.

Sigma-Aldrich, Inc. warrants that its products conform to the information contained in this and other Sigma-Aldrich publications.

Purchaser must determine the suitability of the product(s) for their particular use. Additional terms and conditions may apply.

Please see reverse side of the invoice or packing slip.